

Development of a Beam Trajectory Monitoring System Using e^+/e^- Pair Production Events

Shota KIMURA, Yusaku EMOTO, Kento FUJIHARA, Hiroshi ITO, Hideyuki KAWAI, Atsushi KOBAYASHI, and Takahiro MIZUNO

Abstract—In particle therapy, it is important to monitor the Bragg-peak position. It was simulated by GEANT4 Monte Carlo Simulation Code that the distribution of secondary generated gamma rays on the carbon beam therapy and the proton beam therapy. This simulation shows that gamma rays whose energy is 10 MeV or more are intensively generated at the Bragg-peak position. We are developing the system to monitor the Bragg-peak position which can measure pair production events occurred in the detector by gamma rays from irradiation points. The momentum direction of the gamma ray can be determined by measuring passing points and energy of e^+ and e^- generated by pair production. This system has 5 parts. The first is the conversion part. This part consists of several layers. Each layer is composed of a La-GPS ($(\text{Gd}_{0.75}\text{La}_{0.24}\text{Ce}_{0.01})_2\text{Si}_2\text{O}_7$) scintillator plate and wavelength-shifting fibre (WLSF) sheets. The scintillator plate is sandwiched between sheets, where the directions of the sheets are in orthogonally x and y directions. In this part, gamma rays are converted to e^+ e^- pairs and the position where the conversion occurred is determined. The second is the tracking part. This part consists of 2 layers of scintillating fibre tracker. Each layer has 6 scintillating fibre sheets for x, x', u, u', v, and v'. The third is the energy measurement part. It measures the energy of e^+ and e^- by scintillator array and Silicon Photomultipliers. The fourth is the veto counter for bremsstrahlung gamma rays from e^+ and e^- . The fifth is the beam monitor. By experiment, the number of photoelectrons of La-GPS with a WLSF (B-3(300)MJ, Kuraray) sheet and scintillating fibre (SCSF-78, Kuraray) when charged particle passed was measured as 9.7 and 7.6 respectively.

Index Terms—particle therapy, pair production, Geant4

I. INTRODUCTION

IN particle therapy, cancer cells can be killed by matching the Bragg-peak position and the cancer position. Conversely, if the position of the Bragg-peak deviates from cancer cells even a little, normal cells could be killed. Thus, in particle therapy, it is important to monitor the Bragg-peak position. To monitor the Bragg-peak position, positron emission tomography (PET) detectors [1], Compton cameras [2] have been studied.

We simulated on GEANT4 Monte Carlo Simulation Code that the distribution of secondary generated gamma rays on the carbon beam therapy and the proton beam therapy. The results of proton beam are shown in Fig.1 and parameters of simulations are on Table I. This simulation shows that gamma rays whose energy is 10 MeV or more are intensively generated at the Bragg-peak position. On the other hand, gamma rays whose energy is around 0.511 MeV are widely

distributed in the body. Thus, it is clear that using high energy gamma rays is the best way to monitor the Bragg-peak position.

II. METHODS

Most of the reaction of gamma rays which energy is 10 MeV or more are pair production [3]. The momentum direction of the gamma ray can be determined by measuring passing points and energy of e^+ and e^- generated by pair production. The Bragg-peak position can be determined by obtaining the intersection of the trajectory of the gamma ray and the trajectory of the particle beam.

We are developing the system to monitor the Bragg-peak position which can measure pair production events occurred in the detector by gamma rays from irradiation points. Fig.2 is a schematic diagram of the system. This system has 5 parts. The first is the conversion part. This part consists of several layers. Each layer is composed of a La-GPS ($(\text{Gd}_{0.75}\text{La}_{0.24}\text{Ce}_{0.01})_2\text{Si}_2\text{O}_7$) scintillator plate and wavelength-shifting fibre (WLSF) sheets. The size of the scintillator plate is 300 mm×300 mm×1 mm. The sheets are made by arranging 1500 WLSFs with a diameter of 0.2 mm. The scintillator plate is sandwiched between sheets, where the directions of the sheets are in orthogonally x and y directions. In this part, gamma rays are converted to e^+ e^- pairs and the position where the conversion occurred is determined. The second is the tracking part. This part consists of 2 layers of scintillating fibre tracker. Each layer has 6 scintillating fibre sheets for x, x', u, u', v, and v'. Fig.3 shows construction of the layer. The third is the energy measurement part. It measures the energy of e^+ and e^- by plastic scintillator array and SiPM. Each scintillator is the size of 20 mm×20 mm×100 mm. The fourth is the veto counter for bremsstrahlung gamma rays from e^+ and e^- . This part consists of 60 layers of simplified detectors of conversion part. WLSF sheet is just on the single surface, and WLSFs are connected to the Photomultiplier tube (PMT) collectively. In this part, 99% efficiency is expected. The fifth is the beam monitor. This part is a small version of the tracking part.

We confirmed the basic performance of the system by experiments. We measured the number of photoelectrons when the charged particle pass through La-GPS plate scintillator of 1 mm thickness with a WLSF (B-3(300)MJ, ϕ 0.2 mm, Kuraray) sheet. We also measured the number of photoelectrons when a beta ray from ^{90}Sr source passes through a scintillating fibre (SCSF-78, ϕ 1.0 mm, Kuraray). Just one side of the fibres are connected to the PMTs. Setup of the experiment is on Fig.4.

Shota KIMURA is with the Graduate School of Science, Chiba University, Chiba, 263-8522, Japan (e-mail: shota_kimura@hepburn.s.chiba-u.ac.jp).
Manuscript received the 1st of June, 2017.

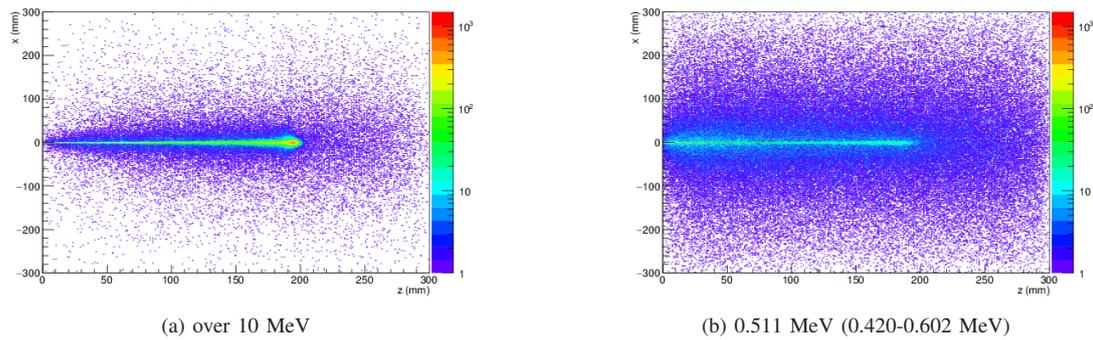


Fig. 1. Simulated results of the distribution of secondarily generated gamma rays' final scattered points on the proton beam therapy. Horizontal axis means the depth of the body, and vertical axis means the vertical position of the body.

TABLE I
PARAMETERS OF THE SIMULATION

| Particle | Proton | Carbon |
|---------------------|---|---------------------------|
| Beam Energy | 175 MeV | 290 MeV/n |
| | QGSP_BIC_HP | FTFP_BERT_HP |
| Physics List | G4RadioactiveDecayPhysics | G4RadioactiveDecayPhysics |
| Material of Phantom | G4_MIX_D_WAX (H: 13.4%, C: 77.8%, O: 3.5%, Mg: 3.9%, Ti: 1.4%) | |

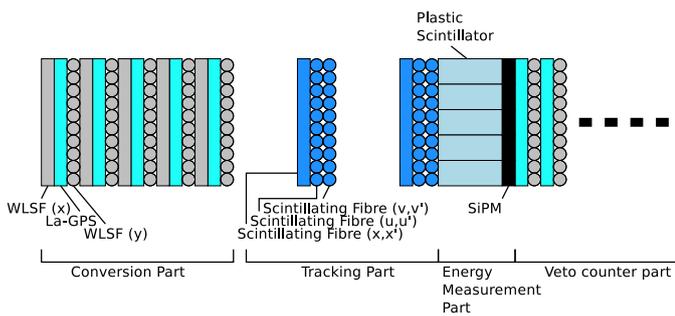


Fig. 2. A schematic diagram of the system

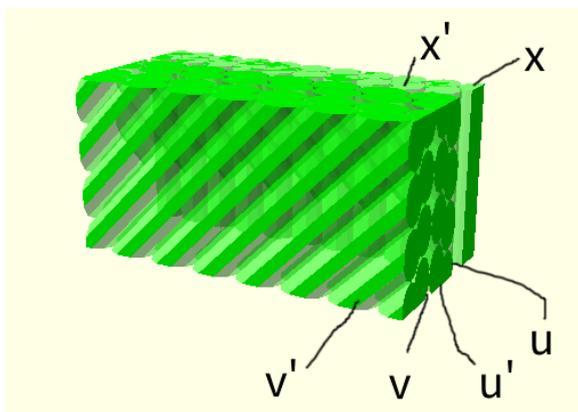


Fig. 3. Construction of scintillating fibre tracker.

III. RESULTS

The number of photoelectrons to 0.511 MeV gamma rays was measured as 14.7 in average [4]. We measured 9.7 photoelectrons in average from a WLSF sheet when a beta

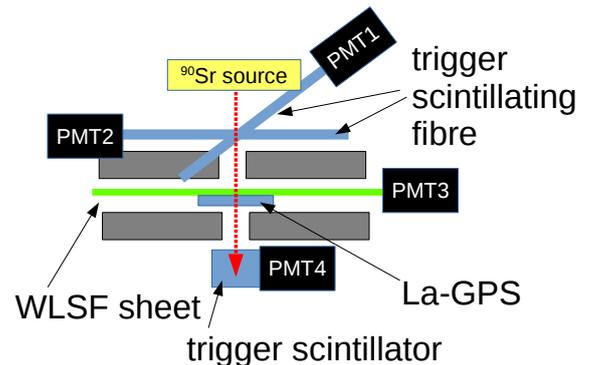


Fig. 4. Setup of the experiment

ray from ^{90}Sr source passes through the La-GPS scintillator plate, and 7.6 photoelectrons in average from a scintillating fibre.

IV. CONCLUSION

The best way to monitor the Bragg-peak position is using gamma ray of several dozen MeV. To monitor with such gamma rays, using pair production events such as our system is the most reasonable. According to the experiment, each component of our system has sufficient amount of luminescence.

REFERENCES

- [1] T. Nishio, T. Ogino, K. Nomura, and H. Uchida, "Dose-volume delivery guided proton therapy using beam on-line pet system," *Medical physics*, vol. 33, no. 11, pp. 4190–4197, 2006.
- [2] S. Peterson, D. Robertson, and J. Polf, "Optimizing a three-stage compton camera for measuring prompt gamma rays emitted during proton radiotherapy," *Physics in medicine and biology*, vol. 55, no. 22, p. 6841, 2010.

- [3] M. Berger, J. Hubbell, S. Seltzer, J. Chang, J. Coursey, R. Sukumar, D. Zucker, and K. Olsen, "Xcom: Photon cross sections database," <https://www.nist.gov/pml/xcom-photon-cross-sections-database>.
- [4] N. KANEKO, "Development of the gamma ray detector with wlsf for pet imaging," Master's thesis, Chiba University, 2016.